


This page explains the results sent to people who had their blood tested for PFCs as part of a legal settlement with Solvay Specialty Polymers USA, L.L.C.

Testing for these chemical is not a standard clinical blood test. As such, this blood test only tells you whether you have these specific chemicals in our blood. At this time these results cannot be used to predict health effects or causally linked to specific health problems.

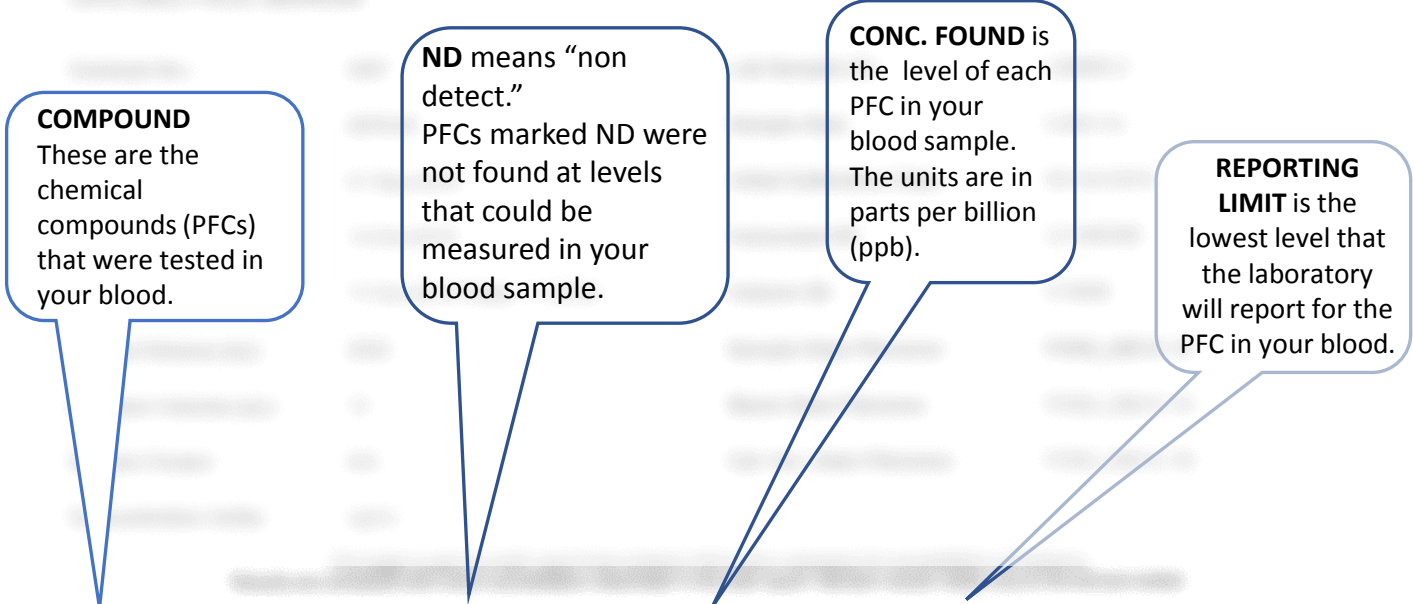

COMPOUND	LAB FLAG ¹	CONC. FOUND	REPORTING LIMIT (RL) ²	RETENTION TIME
PFBA	ND		0.500 (L)	
PFPeA	ND		0.500 (L)	
PFHxA	ND		0.500 (L)	
PFHpA	ND		0.500 (L)	
PFOA		5.88	0.500 (L)	6:15
PFNA		4.61	0.500 (L)	6:38
PFDA	ND		0.500 (L)	
PFUnA	ND		0.500 (L)	
PFDoA	ND		0.500 (L)	
PFBS	ND		1.00 (L)	
PFHxS		2.60	1.00 (L)	6:28
PFOS		6.16	1.00 (L)	
PFOSA	ND		0.500 (L)	7:32

PFNA was the chemical that was found at high levels in the Paulsboro community water supply

RETENTION TIME is part of the lab testing process.